

POSITION CHECK

LED START/STOP Button	Symbol in the display	Description
		• Arm too low, position higher • Release of the thorax not ensured • Therapy not possible
		• Arm to high, position lower • Stamp has no contact with the thorax • Therapy possible, but not recommended
		• Arm adjusted optimally • Full release and configured compression depth can be achieved.

TO THE VIDEOS



**Positioning the
corpuls cpr:**
Further information
and instructions



**Shock synchronisation
with the corpuls cpr:**
Further information
and instructions

UK Distributor:

Ortus Technology | Skyview Business Centre |
9 Churchfield Road | Sudbury | CO10 2YA

Phone +44 (0) 845 459 4705
E-mail hello@ortus.co.uk
Web theortusgroup.com

Manufacturer:

corpuls | GS Elektromedizinische Geräte
G. Stemple GmbH | Hauswiesenstraße 26 |
86916 Kaufering | Germany



This card does not replace the thorough
reading of the User Manual (P/N 09130.02)

Products may not be available in all markets as product availability
depends on the regulatory and/or medical processes in individual
markets. For availability please contact info@corpuls.com.
Printing errors as well as construction and design modification
subject to change. All mentioned product names are registered
trademarks of the respective owners.
P/N 76143.91020 Vers. 2.0 (03/21)




corpuls®



corpuls cpr
POCKET CARD

4-STEP APPROACH

1. PREPARING

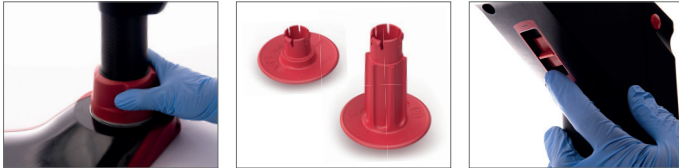

1. Mount the arm on the board
2. Insert a stamp of the correct size
3. Switch on device at the underside of the arm
4. Check therapy parameters on the display
5. Open the locking lever, swivel the arm aside

2. POSITIONING



1. Position the board under the head and neck of the patient
2. Interrupt manual thorax compressions (only minimally!)
3. Lift patient by the shoulders and slide the board under the patient
4. Start manual thorax compressions again



3. ADJUSTING & STARTING



1. Position the **corpuls cpr** stamp in the correct area on the thorax (see below)
2. When „green“, close locking lever and start therapy (Start-/Stop Button)


4. PREPARING TRANSPORT



- Attach the fixation ring with the straps and pull tight

CORRECT STAMP POSITION

- Position the stamp in the **middle of the lower part of the sternum**
- Never position the stamp on or below the xiphoid process



INTERRUPT THORAX COMPRESSIONS ONLY MINIMALLY!

